

EU Type Examination Certificate Number: 0120/SGS0206

## Zhejiang Eastron Electronic Co.,Ltd.

No. 1369, Chengnan Road, Jiaxing, Zhejiang, China, 314001.

Instrument Identification: SDM230 Series

Instrument Traceable Number 0120/SGS0206

Single Phase, Active Import/ Export (kWh), Indoor, Electricity Meter

has been assessed and certified as meeting the requirements of

# **EU Directive 2014/32/EU**

on Measuring Instruments Annex II, Module B

It is certified that the manufacturer's technical design and specimen for the above instrument has been examined and, based on the evidence submitted, it is considered that the instrument conforms to the requirements of Annex V of EU Directive 2014/32/EU

This certificate must be used in conjunction with a certificate covering the product verification as required in Annex II, Module D or Annex II, Module F

This certificate is valid for 10 years from 30<sup>th</sup> September 2015 to 29<sup>th</sup> September 2025 Issue 4

> Certification is based on report number(s) SHES141200649301 issued 16<sup>th</sup> April 2015 EMA207767 issued 9<sup>th</sup> October 2015

> > **Authorised Signature**

SGS United Kingdom Limited, Notified Body 0120 Unit 202B Worle Parkway, Weston-super-Mare, BS22 6WA□UK t +44 (0)1934 522917 f +44 (0)1934 522137 www.sgs.com

Contact Address SGS United Kingdom Ltd, Units 12A & 12B, South Industrial Estate, Bowburn, Durham, DH6 5AD UK
t +44 (0)191 377 2000 f +44 (0)191 377 2020 www.sgs.com



# 0120/SGS0206

Issue Number: 4 Dated: 29<sup>th</sup> November 2018

#### 1. Technical Data


Manufacturer	Zhoijang Egetran Electronic Co. Ltd.			
Manufacturer	Zhejiang Eastron Electronic Co.,Ltd			
Meter Type(s)	SDM230-Modbus, SDM230-Bi, SDM230-DR,SDM230-Pulse, SDM230-Mbus V1, SDM230-Mbus V2, SDM230-2T			
Voltage Rating (Un)	230V			
Current Rating (Imin – Iref (Imax))	0.5-10(100)A			
Frequency (Fn)	50Hz			
Active Accuracy Class (kWh)	A or B (kWh)			
Type of circuit	1p2w			
Temperature Range	-25°C to +55°C			
Software Version No's	SDM230-Modbus, SDM230-Bi, SDM230-DR, SDM230-Pulse:V1.2 SDM230-2T: V1.3 SDM230-Mbus V1, SDM230-Mbus V2: V1.4			
Checksum No's	SDM230-Modbus, SDM230-Bi, SDM230-DR, SDM230-Pulse, SDM230-Mbus: 0x000052F2 SDM230-2T: 0x00001AD5 SDM230-Mbus V1, SDM230-Mbus V2: 0x00004D23			
Identification Location	Nameplate			
Bill Of Materials No.'s	SDM230-Modbus, SDM230 Bi, SDM230 DR, SDM230 Pulse: 20150929 SDM230-2T: DH-JS-180009-1.0 SDM230-Mbus: DH-JS-180017-V1.0 SDM230-Mbus V2: DH-JS-180029-V1.0			
IP Rating	IP51			
Insulation Protective Class	Class II			
LED Pulse Constant	1000imp/ kWh			
Impulse Voltage Rating	6kV			
AC Voltage Rating	4kV			
Terminal Cover Sealing Type	4 x Wire & Crimp			
Integrity of meter	Inaccessible without breaking seals			
Intended Location of the Meter	Indoor			
Type of Register	LCD			



# 0120/SGS0206

Issue Number: 4 Dated: 29<sup>th</sup> November 2018

#### 2. Photograph of Meter and Sealing Plan

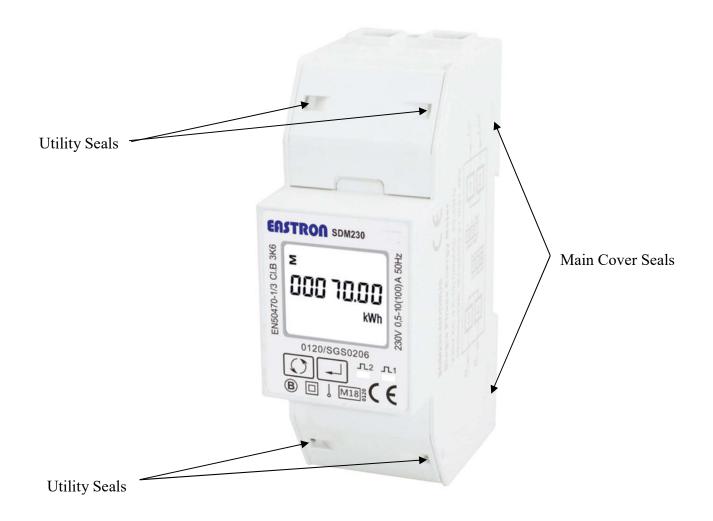




## 0120/SGS0206

Issue Number: 4 Dated: 29<sup>th</sup> November 2018

#### 3. Nameplates and Markings




















## 0120/SGS0206

Issue Number: 4 Dated: 29<sup>th</sup> November 2018















## 0120/SGS0206

Issue Number: 4 Dated: 29<sup>th</sup> November 2018

#### 4. Influence factors for temperature, frequency and voltage

During the type approval examination the influence factors for temperature, frequency and voltage are determined per load point. The table above represents the sum of the square values per load, determined via the following formula:-

$$\delta e(T, U, f) = \sqrt{(\delta e^2(T, I, \cos\varphi), \delta e^2(U, I, \cos\varphi), \delta e^2(f, I, \cos\varphi))}$$

#### where

 $\delta e(T, I, \cos \varphi) =$  Additional error due to variation of the temperature at the same load  $\delta e(U, I, \cos \varphi) =$  Additional error due to variation of the voltage at the same load  $\delta e(f, I, \cos \varphi) =$  Additional error due to variation of the frequency at the same load

Current	PF Cos	-25°C	-10°C	5°C	30°C	40°C	55°C
Imin	1.0	0.45	0.33	0.23	0.15	0.17	0.23
Itr	1.0	0.44	0.31	0.19	0.07	0.10	0.18
10ltr	1.0	0.42	0.29	0.18	0.03	0.08	0.16
Imax	1.0	0.27	0.19	0.12	0.03	0.06	0.12
Itr	0.5ind	0.48	0.36	0.27	0.17	0.18	0.22
10ltr	0.5ind	0.41	0.28	0.17	0.03	0.08	0.17
Imax	0.5ind	0.27	0.18	0.12	0.04	0.07	0.13
Itr	0.8cap	0.45	0.31	0.20	0.09	0.12	0.18
10ltr	0.8cap	0.40	0.27	0.16	0.04	0.10	0.19
Imax	0.8cap	0.26	0.19	0.11	0.05	0.08	0.15

DU\_CST-ME-002 Rev 2 EU Type Examination Cert.



### 0120/SGS0206

Issue Number: 4 Dated: 29<sup>th</sup> November 2018

#### 5. Annex of Variants

**Product Variant Identification Details:** 

**Type Designation Description of meter** SDM230-Modbus: Single tariff, total active energy, resettable active energy, import active energy, export active energy, total reactive energy, import reactive energy, export reactive energy, active power, reactive power, voltage, current, frequency, power factor, power demand, RS485 Modbus communication SDM230-Mbus Single tariff, total active energy, resettable active energy, import active energy, export active energy, total reactive energy, import reactive energy, export reactive energy, active power, reactive power, voltage, current, frequency, power factor, power demand, Mbus communication SDM230-Pulse: Single tariff, total active energy, resettable active energy, import active energy, export active energy total reactive energy import reactive energy export reactive energy active, power reactive, power, voltage, current, frequency, power factor, power demand. SDM230-DR: Single tariff, total active energy, resettable energy, active power SDM230-Bi: Single tariff, import active energy, export active energy, import active power, export active power, total active energy, total active power SDM230-2T: Two tariff, total active energy, resettable active energy, import active energy, export active energy, total reactive energy, import reactive energy, export reactive energy, active power, reactive power, voltage, current, frequency,

Modifications to the meter(s) described according to approval No.0120/SGS0206 must be notified to the issuing body to confirm the meter(s) continuing compliance to the relevant pattern approval standard(s).

power factor, power demand, RS485 Modbus communication



## 0120/SGS0206

Issue Number: 4 Dated: 29<sup>th</sup> November 2018

#### 6. Document Revision History

Issue	Date	Comments
1	09/10/2015	Initial Issue
2	23/11/2015	Meter types SDM230-Pulse, SDM230-DR and SDM230-Bi added to approval
3	06/06/2018	Meter type SDM230-2T and SDM230-Mbus added to approval
4	29/11/2018	Meter type SDM230-Mbus V2 added to approval

This document is issued by the Company subject to its General Conditions for Certification Services, available on request or accessible at <a href="http://www.sgs.com/en/Terms-and-Conditions.aspx">http://www.sgs.com/en/Terms-and-Conditions.aspx</a>.

Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 28 days only.

**END OF CERTIFICATE**